

IB/2005/050405

REC'D 03 FEB 2005

WIPO

PA 1274029

# THE UNITED STATES OF AMERICA

TO ALL TO WHOM THESE PRESENTS SHALL COME:

UNITED STATES DEPARTMENT OF COMMERCE

United States Patent and Trademark Office

January 21, 2005

THIS IS TO CERTIFY THAT ANNEXED HERETO IS A TRUE COPY FROM THE RECORDS OF THE UNITED STATES PATENT AND TRADEMARK OFFICE OF THOSE PAPERS OF THE BELOW IDENTIFIED PATENT APPLICATION THAT MET THE REQUIREMENTS TO BE GRANTED A FILING DATE UNDER 35 USC 111.


APPLICATION NUMBER: 60/542,793 ✓

FILING DATE: February 06, 2004 ✓

## PRIORITY DOCUMENT

SUBMITTED OR TRANSMITTED IN  
COMPLIANCE WITH RULE 17.1(a) OR (b)

By Authority of the  
COMMISSIONER OF PATENTS AND TRADEMARKS

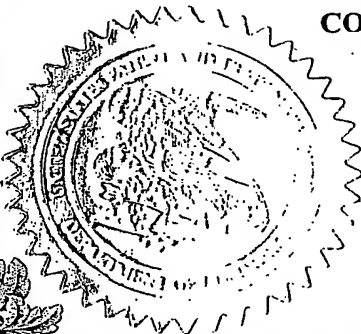

P. SWAIN

Certifying Officer

17281 U.S. PTO

Please type a plus sign (+) inside this box → ☒

Under the Paperwork Reduction Act of 1995, no persons are required to respond to a collection of information unless it displays a valid OMB control number.

PTO/SB/16 (02-01)  
Approved for use through 10/31/2002. OMB 0851-0032  
U.S. Patent and Trademark Office; U.S. DEPARTMENT OF COMMERCE

## PROVISIONAL APPLICATION FOR PATENT COVER SHEET

This is a request for filing a PROVISIONAL APPLICATION FOR PATENT under 37 CFR 1.53(c).

Express Mail Label No. EU778901050US

031491 U.S. PTO  
60/542793



020604

INVENTOR(S)					
Given Name (first and middle (if any))	Family Name or Surname	Residence (City and either State or Foreign Country)			
John	Murkowski	Seattle, WA			
Robert	Mesaros	Bothell, WA			
Larry	Azzano	Seattle, WA			
<input type="checkbox"/> Additional inventors are being named on the _____ separately numbered sheets attached hereto					
TITLE OF THE INVENTION (280 characters max)					
DIAGNOSTIC ULTRASOUND SYSTEM WITH ARTICULATING FLAT PANEL DISPLAY					
Direct all correspondence to: CORRESPONDENCE ADDRESS					
<input checked="" type="checkbox"/> Customer Number		28159		<div style="border: 1px solid black; padding: 5px;">Place Customer Number Bar Code Label here</div>	
OR Type Customer Number here					
<input type="checkbox"/> Firm or Individual Name		W. Brinton Yorks, Jr.			
Address					
Address					
City		State		ZIP	
Country		Telephone	425-487-7152	Fax	
ENCLOSED APPLICATION PARTS (check all that apply)					
<input checked="" type="checkbox"/> Specification Number of Pages		17		<input type="checkbox"/> CD(s), Number	
<input checked="" type="checkbox"/> Drawing(s) Number of Sheets		12		<input checked="" type="checkbox"/> Other (specify)	
<input type="checkbox"/> Application Data Sheet. See 37 CFR 1.76					
METHOD OF PAYMENT OF FILING FEES FOR THIS PROVISIONAL APPLICATION FOR PATENT					
<input type="checkbox"/> Applicant claims small entity status. See 37 CFR 1.27.				FILING FEE AMOUNT (\$)	
<input type="checkbox"/> A check or money order is enclosed to cover the filing fees				160.00	
<input checked="" type="checkbox"/> The Commissioner is hereby authorized to charge filing fees or credit any overpayment to Deposit Account Number:		14-1270			
<input type="checkbox"/> Payment by credit card. Form PTO-2038 is attached.					
The invention was made by an agency of the United States Government or under a contract with an agency of the United States Government.					
<input checked="" type="checkbox"/> No.					
<input type="checkbox"/> Yes, the name of the U.S. Government agency and the Government contract number are: _____					

Respectfully submitted,

SIGNATURE

*W. Brinton Yorks, Jr.*

TYPED or PRINTED NAME

W. Brinton Yorks, Jr.

TELEPHONE

425-487-7152

Date

Feb. 6, '04

REGISTRATION NO.  
(if appropriate)  
Docket Number:

28,923

PHUS040118

## USE ONLY FOR FILING A PROVISIONAL APPLICATION FOR PATENT

This collection of information is required by 37 CFR 1.51. The information is used by the public to file (and by the PTO to process) a provisional application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 8 hours to complete, including gathering, preparing, and submitting the complete provisional application to the PTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, Washington, D.C. 20231. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Box Provisional Application, Assistant Commissioner for Patents, Washington, D.C. 20231.

PHUS040118

IN THE UNITED STATES  
PATENT AND TRADEMARK OFFICE

APPLICANT(S): John Murkowski; Robert Mesaros; Larry Azzano

FOR: "Diagnostic Ultrasound System With Articulating Flat Panel  
Display"


EXPRESS MAIL CERTIFICATE

"Express Mail" Mailing number: EU778901050US

Date of Deposit: February 6, 2004

I hereby certify that this provisional application, including 17 pages of specification and 12 pages of drawings, is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 on the date indicated above and is addressed to the Commissioner of Patents, Mail Stop: Provisional Application, P. O. Box 1450, Alexandria, VA 22313-1450.

Jill Anne Peistrup

  
(Signature of person mailing paper or fee)

DIAGNOSTIC ULTRASOUND SYSTEM WITH  
ARTICULATING FLAT PANEL DISPLAY

5 This invention relates to medical diagnostic  
imaging systems and, in particular, to ultrasonic  
diagnostic imaging systems with flat panel displays  
that can be easily positioned for viewing by a user.

10 Ultrasound systems are now being designed to be  
more ergonomically comfortable for the user to  
operate. Often, the ultrasound system is wheeled to  
the patient's bedside for imaging. The sonographer  
must then be able to hold the probe in contact with  
the patient while operating the ultrasound system  
controls and viewing the images produced on the  
15 system image display. To enable the sonographer to  
assume a comfortable position while doing this, one  
which is primarily focused on the patient, it is  
desirable for the system controls and display to be  
movable to a comfortable operating and viewing  
20 position. For instance, US pat. 6,669,639 (Miller et  
al.) describes the ultrasound system shown in FIGURE  
1. The display monitor 20 of this system is mounted  
on a 2-arm articulating mount 30 on the upper surface  
of the system cart 12, which enables the monitor to  
25 be moved from side to side of the ultrasound system  
cart and to be rotated toward the sonographer or  
patient for easy viewing. US pat. [application  
serial number 10/155,459, entitled "DIAGNOSTIC  
ULTRASOUND SYSTEM CART WITH LATERALLY ARTICULATING  
30 CONTROL PANEL,"] describes the ultrasound system  
shown in FIGURE 2, which uses a flat panel display 16  
mounted at a nominal position above the system  
control panel 18. The control panel 18 of this  
system can move from one side of the system cart to  
35 the other and can rotate or swivel toward the

ATL-358

sonographer for comfortable bedside operation. It would be desirable for the flat panel display 16 to be similarly movable to a comfortable viewing position. An optimal design would enable the display 5 16 to be positioned over a wide range of lateral viewing positions and heights, and to be easy for the sonographer to reposition with one hand.

In accordance with the principles of the present invention an ultrasound system is described with a 10 flat panel display that articulates to be viewed over a wide range of viewing positions. The articulation is provided by a 2-arm articulation system with a counter-weight assisted 4-bar linkage. The counter-weight assist and the 4-bar linkage require very 15 little effort to reposition the display to a comfortable viewing position. The flat panel display has a peripheral gripping surface which enables the display to be held and repositioned with one hand so that the display can be easily adjusted to be 20 viewable by either the sonographer or the patient.

In the drawings:

FIGURE 1 illustrates a cart-borne ultrasound with an articulating monitor.

FIGURE 2 illustrates a cart-borne ultrasound 25 system with a flat panel display and an articulating control panel.

FIGURE 3 illustrates an articulating flat panel display for an ultrasound system constructed in accordance with the principles of the present 30 invention.

FIGURE 4 are forward and rearward perspective views of an articulating flat panel display of the present invention.

FIGURE 5 illustrates a flat panel display with a 35 peripheral gripping surface for articulation.

ATL-358

FIGURE 6 is a partially cutaway view of the flat panel display of FIGURE 5, showing the back gripping surface.

5        FIGURES 7a and 7b are cross-sectional views of the flat panel display of FIGURE 5.

FIGURE 8a, 8b and 8c illustrate an articulating flat panel display of the present invention in the raised, nominal, and stowed positions.

10       FIGURE 9 illustrates the range of articulation of an articulating flat panel display of the present invention in a vertical plane.

FIGURES 10a, 10b, and 10c illustrate the lateral range of articulation of an articulating flat panel display of the present invention.

15       FIGURE 11 is an illustration of a number of laterally articulated positions of an articulating flat panel display of the present invention.

20       FIGURE 12 illustrates a cart-borne ultrasound system of the present invention with a laterally articulating control panel and an articulating flat panel display.

Referring now to FIGURE 3, an articulating flat panel display assembly constructed in accordance with the principles of the present invention is shown.  
25       The flat panel display 40 has a viewing screen 42 which is enclosed in an enclosure having a front bezel 44 which surrounds the edges of the display in the front and a rear enclosure section 46. The front bezel 44 and the periphery of the rear enclosure  
30       section 46 include gripping surfaces by which a user can grip the flat panel display to adjust its position. The flat panel display 40 is mounted to the ultrasound system by an articulating arm assembly 50. The lower arm or main base 52 has a mounting end  
35       60 which is mounted to the ultrasound system. The

main base 52 is pivotally mounted to the ultrasound system to pivot about a vertical pivot axis extending through the mounting end 60. The mounting end 60 encloses a circular mounting bracket with a tooth  
5 that rides in a circular slot inside the mounting end 60. The circular slot extends only halfway around the pivot axis of the mounting end and thereby restrains the range of pivoting of the mounting end to 180°. It is desirable to prevent continuous  
10 unlimited rotation of the lower arm because the cables to the flat panel display extend through the articulating arms. Continuous rotation of the arms would cause these cables to become twisted and ultimately to be damaged.

15 The main base 52 of the articulating arm assembly 50 is angled upward at a fixed angle of approximately 25°. This upward angling of the main base 52 provides elevation for the upper arm and flat panel above the upper surface of the ultrasound  
20 system. This elevation provides clearance above parts or accessories of the system that may be located above or placed on the upper surface of the system. The elevation also raises the upper arm to a level where it will locate the flat panel display in  
25 a nominal, neutrally balanced viewing position when the upper arm is oriented horizontally.

The upper end 62 of the main base 52 mates with the elbow 64 of the upper arm 54. The elbow 64 and upper end 62 are pivotally connected so that the  
30 elbow joint will pivot about a second vertical axis. The upper end 62 of the main base includes a pin which rides in a groove in the inner sleeve of the elbow. The pin and groove of this pivoting connection function in the same manner as the tooth  
35 and circular slot of the mounting end 60, allowing

ATL-358

the two arms to rotate through a limited arc of the circular 180° groove. The elbow rotation is thus prevented from unlimited rotation which could damage the flat panel cables.

5       The upper arm 54 includes a 4-bar linkage 70. The four bars 72, 74, 76 and 78 of the linkage 70 are pivotally connected by pivot pins a and b at the forward end of the arm 54 and by pivot pins c and d at the elbow end of the arm. The 4-bar linkage 70  
10 enables the flat panel display to be raised and lowered with respect to the elbow 64. When the upper arm 54 is viewed from the side, the ends of the pivot pins a, b, c, and d will always form a parallelogram as the linkage is articulated up and down. The two  
15 upper bars 72 and 74 of the linkage 70 are in this embodiment formed by the two sides of a U-shaped steel plate. The use of the steel plate for the two upper bars provide strength and rigidity between the two bars. The two lower bars 76 and 78 in this  
20 embodiment are formed by separate bars which are connected by ribs 82 for strength and rigidity between the lower bars.

25       Contained within the four bars of the 4-bar linkage 70, in addition to the cabling to the flat panel display, is a pneumatic shock or piston 56. The compressive force of the piston 56 provides a counter-weight to the weight of the flat panel display. The pneumatic piston 56 is pivotally  
30 connected to a tilt/swivel base 102 at one end of the upper arm 54, and is also pivotally connected to the elbow 64 at the other end of the upper arm 54. The pivot connection at the elbow 64 is mounted on a threaded shaft vertically positioned in the elbow 64. A hole 66 in the elbow 64 provides access to the hex-  
35 shaped head of the threaded shaft. As the threaded

ATL-358



shaft is turned the pivot connection of the pneumatic piston will move up or down in relation to the c and d pivots of the 4-bar linkage. This repositioning of the elbow end of the piston will increase or decrease the tension or stiffness of the force provided by the piston. When the piston force is made stiffer, the user will have to use more force to move the flat panel display down and less force to move the display up. When the piston force is made less stiff, the user will be able to use less force to move the display down and more force to move the display up.

The tilt/swivel base 102 is pivotally connected to a tilt/swivel bracket 104. This connection permits the bracket 104 to rotate about a vertical axis passing through the base 102 and bracket 104, enabling the flat panel display to be turned from side to side without repositioning the articulating arm assembly 50. The tilt/swivel bracket 104 is pivotally mounted to the rear enclosure 46 of the flat panel display by a pivot connection 106 which pivots around a horizontal pivot axis. This pivot axis permits the flat panel display to be tilted to face upward or downward without moving the articulating arm assembly.

Extending downward from the bottom of the upper articulating arm 54 is a catch plate 92. The catch plate 92 will engage a spring-loaded lock plate 94 in the lower arm 52 when the two arms are brought together. The catch plate 92 will contact a spring-loaded ball which is partially visible to the right of the lock plate 94 when the lock is open, which causes the lock plate 94 to spring to the right and retain the catch plate 92. A lock release 96 on the bottom of the lower arm will then move to the locked position. The two arms will remain locked together

ATL-358

until the lock release 96 is moved to the unlock position, which moves the lock plate 94 to the left and releases the engaged catch plate 92. The two arms are locked together to secure the articulating display and prevent articulation when the ultrasound system is being moved or transported.

FIGURE 4a is a perspective view of the articulating flat panel display when the 4-bar linkage upper arm 54 is raised above the horizontal to elevate the display to a higher viewing position. FIGURE 4b is a view of the same positioning of the articulating display from the rear of the flat panel display. As the arrows in FIGURE 4b indicate, the flat panel display can be repositioned horizontally by operation of the vertical axis pivots of the assembly, and the flat panel display can be moved vertically by movement of the bars of the 4-bar linkage 70.

FIGURE 5 shows a front view of a flat panel display embodying a further aspect of the present invention. FIGURE 1 shows the monitor 20 of the system 10 there shown with a handle 100 on the front of the monitor. The monitor can be repositioned by grasping the handle to move the monitor. A flat panel display, lacking the weight of the glass of a display monitor, does not require a repositioning means as robust as a handle. In the embodiment of FIGURE 5 the bezel 44 around the front of the display screen 42 has a surface designed to be gripped by the user's thumb when repositioning the flat panel display. This gripping surface can be provided by forming the front bezel 44 of a silicon or rubber-like material. In a constructed embodiment the gripping surface is formed by coating a bezel formed of hard plastic with a thermoplastic elastomeric

ATL-358

coating such as a Sanopreen overmold or Soft-touch spray coating available from Also Corp. of Vernon, California, USA. FIGURE 6 is a partially cutaway perspective view of the flat panel display 40 which better illustrates the curvature of the bezel 44 which provides a contoured surface that can be gripped firmly with the user's thumb without slipping. Also visible in the cutaway view is the periphery of the rear enclosure section 46 which also contains a gripping surface for the user's fingers. This gripping surface is provided by the texturing of the surface of the periphery of the section 46. In this case the texturing is provided by perforations 48 through the section 46. These perforations not only provide a good gripping surface on the back periphery of the flat panel display, but also provide ventilation of the flat panel enclosure. FIGURE 7a is a cross-sectional view of the flat panel display which shows the contour of the bezel 44 on the front and the perforations 48 around the rear periphery of the display. FIGURE 7b is a simplification of FIGURE 7a which clearly shows the contoured gripping surface 44 on the front of the flat panel display and the perforated gripping surface 48 on the rear enclosure section 46. One skilled in the art will appreciate that texturing other than perforations may be employed, such as grooves, protrusions, or a roughened surface for gripping.

FIGURES 8a-8c illustrate several vertical articulation positions of an embodiment of the present invention. In a constructed embodiment the surface 100 of the ultrasound system on which the articulating flat panel display is mounted is at a height relative to the control panel such that a nominal display position is provided when the upper

ATL-358

arm 54 is horizontally oriented as shown in FIGURE 8b. The threaded adjustment of the piston 56 is set so that the piston force will offset the weight of the upper arm 54 and the flat panel 40 when the upper arm 54 is in this horizontal position. The upper arm 54 can then be raised and lowered from this nominal position as indicated by the arrows in the drawing, with the piston force continuously providing a balancing counter-weight force. This is due to the use of the 4-bar linkage 70 and the pneumatic shock 56 for the upper arm 54. If the 4-bar linkage were located in the lower arm 52, for instance, there would be a greater disparity between the force required to raise the display and the force required to lower the display. By locating the 4-bar linkage and piston in the upper arm 54, these forces can be more uniformly balanced.

FIGURE 8c shows the articulating arm assembly when the flat panel display is stowed for travel. The upper arm 54 is lowered as indicated by the arrow until the catch plate 92 engages the lock plate 94, which causes the lock to engage and retain the two arms in the illustrated stowed position.

FIGURE 9 illustrates the range of locations in a vertical plane which the flat panel display 40 can assume by use of the articulating arm assembly of FIGURE 3. As the arrows indicate the display 40 can move vertically up or down by reason of the articulation of the 4-bar linkage 70 of the upper arm 54. When the articulating arms are pivoted about their vertical pivot axes, the flat panel display can be repositioned from side to side as indicated by the arrows on either side of the display 40.

FIGURES 10a-10c illustrate the lateral articulation provided by the vertical pivot axes of

ATL-358

the embodiment of FIGURE 3. The pivot axis 122 passes through the mounting end 60 of the lower arm 52, the pivot axis 124 passes through the elbow 64 of the articulating arms, and the pivot axis 126 passes through the tilt/swivel base 102 at the back of the flat panel display 40. As explained previously, the pivoting of the lower arm 52 about the axis 122 is constrained to 180° as shown by arrows 152. The pivoting of the upper arm 54 about the axis 124 is also constrained to 180° as shown by the arrows 154. The flat panel display 40 can pivot over the full range about the end of the upper arm 54 as shown by the arrows 156. In FIGURE 10a the lower arm 52 is in its "home" position in which it extends to the rear of the ultrasound system and the upper arm 54 has been pivoted 90° to the right. The flat panel display has been pivoted about axis 126 to face forward. This, and the orientations of the other two drawings on this sheet, show how the flat panel display may be positioned when the sonographer is diagnosing a patient located on the right side of the ultrasound system. In FIGURE 10b the flat panel display has been brought forward and slightly more to the right by pivoting the lower arm 52 about axis 122 and adjusting the flat panel display about axis 126. In FIGURE 10c the flat panel display is moved toward the center of the ultrasound system by movement about all three axes from the position shown in FIGURE 10b.

FIGURE 11 shows an embodiment of the present invention with a wide range of lateral display positions. Shown in bold in the center of FIGURE 11 is a flat panel display 40 and articulating arm assembly 50 with their arms in the nominal home position. The display screen is facing to the front of the ultrasound system, the lower articulating arm

extends toward the rear of the ultrasound system and the upper articulating arm extends from the elbow with the lower arm at the rear to the front of the ultrasound system. Shown in shadow are many of the positions around the mounting point of the articulating arm assembly in which the flat panel display can be located. As the positions at the top of the drawing illustrate, the flat panel display can even be moved to face to the rear of the ultrasound system, should that become desirable.

FIGURE 12 illustrates an embodiment of the present invention in which the ultrasound system has both an articulating flat panel display 40 and an articulating control panel 18, both of which can be repositioned laterally with respect to the main body 12 of the ultrasound system cart. The flat panel display may be articulated as described in any of the articulating arm embodiments described above, or by means of other articulating mechanisms. The control panel 18 may be articulated laterally such as described in US pat. [application serial number 10/155,459], the contents of which are incorporated herein by reference. With the ability to articulate both the flat panel display 40 and the control panel, the sonographer can configure the ultrasound system to scan a patient in the utmost of comfort and convenience.

ATL-358

WHAT IS CLAIMED IS:

1. An ultrasonic diagnostic imaging system including a main body housing imaging electronics and a control panel coupled to the imaging electronics comprising:
  - a flat panel display electrically coupled to the imaging electronics; and
  - an articulating arm assembly to which the flat panel display is connected for adjusting the viewing position of the flat panel display, the articulating arm assembly including a first arm movably mounted to the main body and a second arm movably connected to the first arm and to the flat panel display, wherein at least one of the arms includes a 4-bar linkage.
2. The ultrasonic diagnostic imaging system of Claim 1, further comprising a wheeled cart on which the main body is mounted.
3. The ultrasonic diagnostic imaging system of Claim 1, wherein the second arm includes a 4-bar linkage.
4. The ultrasonic diagnostic imaging system of Claim 3, wherein the 4-bar linkage includes first and second pivot axes located at an end of the second arm which is connected to the first arm, and third and fourth pivot axes located at an end of the second arm which is connected to the flat panel display.
5. The ultrasonic diagnostic imaging system of Claim 1, further comprising an inter-arm locking mechanism, located on the first and second arms, which acts to lock the two arms together, thereby

ATL-358

restricting relative motion between the two arms.

5       6.    The ultrasonic diagnostic imaging system of Claim 5, wherein the locking mechanism further comprises a user-operated lock release which is operated to cause the locking of the two arms to be released.

10       7.    The ultrasonic diagnostic imaging system of Claim 1, wherein the articulating arm assembly further includes a first vertical pivot axis located at an end of the first arm which is movably mounted to the first body, and a second vertical pivot axis located at an end of the first arm which is connected  
15       to the second arm.

20       8.    The ultrasonic diagnostic imaging system of Claim 7, wherein the articulating arm assembly further includes a third vertical pivot axis located at an end of the second arm which is connected to the flat panel display, and a horizontal pivot axis located at the end of the second arm which is connected to the flat panel display.

25       9.    The ultrasonic diagnostic imaging system of Claim 7, wherein the arc of travel of the first arm about the first vertical pivot axis is constrained to be less than 360°, and wherein the arc of travel of the second arm about the second vertical axis is  
30       constrained to be less than 360°.

35       10.   The ultrasonic diagnostic imaging system of Claim 1, wherein the second arm includes a 4-bar linkage, and wherein the second arm further includes: a pneumatic piston which acts to provide a force

ATL-358



which at least partially offsets the weight of the flat panel display.

5           11. The ultrasonic diagnostic imaging system of Claim 10, further comprising an adjustment mechanism, coupled to the pneumatic piston, which is operable to adjust the force provided by the pneumatic piston.

10           12. The ultrasonic diagnostic imaging system of Claim 11, wherein the pneumatic piston is adjusted to provide a balancing counter-weight force when the second arm is oriented in a horizontal orientation.

15           13. The ultrasonic diagnostic imaging system of Claim 1, wherein the first arm exhibits a fixed upward inclination from an end which is connected to the main body to a second end which is elevated above the connection to the main body, and the second arm includes a 4-bar linkage.

20           14. The ultrasonic diagnostic imaging system of Claim 3, wherein the 4-bar linkage includes first and second upper bars coupled between the first and third pivot axes and third and fourth lower bars coupled  
25           between the second and fourth pivot axes,

          wherein the first bar is rigidly connected to the second bar and the third bar is rigidly connected to the fourth bar.

30           15. An ultrasonic diagnostic imaging system having a main body housing imaging electronics comprising:

          a flat panel display electrically coupled to the imaging electronics; and  
35           an articulating arm assembly coupled to the flat

ATL-358

panel display to enable repositioning of the flat panel display, the articulating arm assembly including:

- 5 a first arm exhibiting a fixed inclination from a first mounting end and a second joint end; and
- a second arm exhibiting a variable inclination from a first end which is coupled to the second joint end of the first arm, and a second end which is coupled to the flat panel display.

10

16. The ultrasonic diagnostic imaging system of Claim 15, wherein the second arm includes a 4-bar linkage which provides the second arm with the variable inclination.

15

17. The ultrasonic diagnostic imaging system of Claim 15, further comprising a first pivot axis located at the first mounting end of the first arm; a second pivot axis located at the second joint end of the first arm, and a third pivot axis located at the second end of the second arm.

20

18. An ultrasonic diagnostic imaging system including a wheeled cart and a main body housing imaging electronics and located on the wheeled cart comprising:

25

- a control panel located on the wheeled cart and electrically connected to the imaging electronics, the control panel being laterally articulable;
- 30 a flat panel display electrically coupled to the imaging electronics; and
- an articulation mechanism, having a mounting end coupled to the wheeled cart or main body and a second end coupled to the flat panel display, and operable to laterally reposition the viewing position of the

35

ATL-358

flat panel display.

19. The ultrasonic diagnostic imaging system of  
Claim 18, wherein the articulating mechanism includes  
5 first and second articulating arms, at least one of  
which includes a 4-bar linkage.

20. The ultrasonic diagnostic imaging system of  
Claim 18, wherein the articulation mechanism further  
10 includes a plurality of vertical pivot axes which  
enable lateral articulation of the flat panel  
display, and a 4-bar linkage which enables vertical  
articulation of the flat panel display.

15

ATL-358

DIAGNOSTIC ULTRASOUND SYSTEM WITH  
ARTICULATING FLAT PANEL DISPLAY


Abstract of the disclosure:

5


10 An ultrasonic diagnostic imaging system includes  
a flat panel display for viewing images produced by  
the ultrasound system. The flat panel display is  
mounted to the ultrasound system by an articulating  
arm assembly having a lower arm with a fixed  
elevation pivotally connected to the ultrasound  
system and an upper arm pivotally connected to the  
lower arm at one end and pivotally connected to the  
flat panel display at the other end. The upper arm  
15 includes a 4-bar linkage which enables the flat panel  
display to be raised and lowered, and a pneumatic  
piston which provides a counter-weight to the weight  
of the flat panel display.

ATL-358


**FIG. 1**

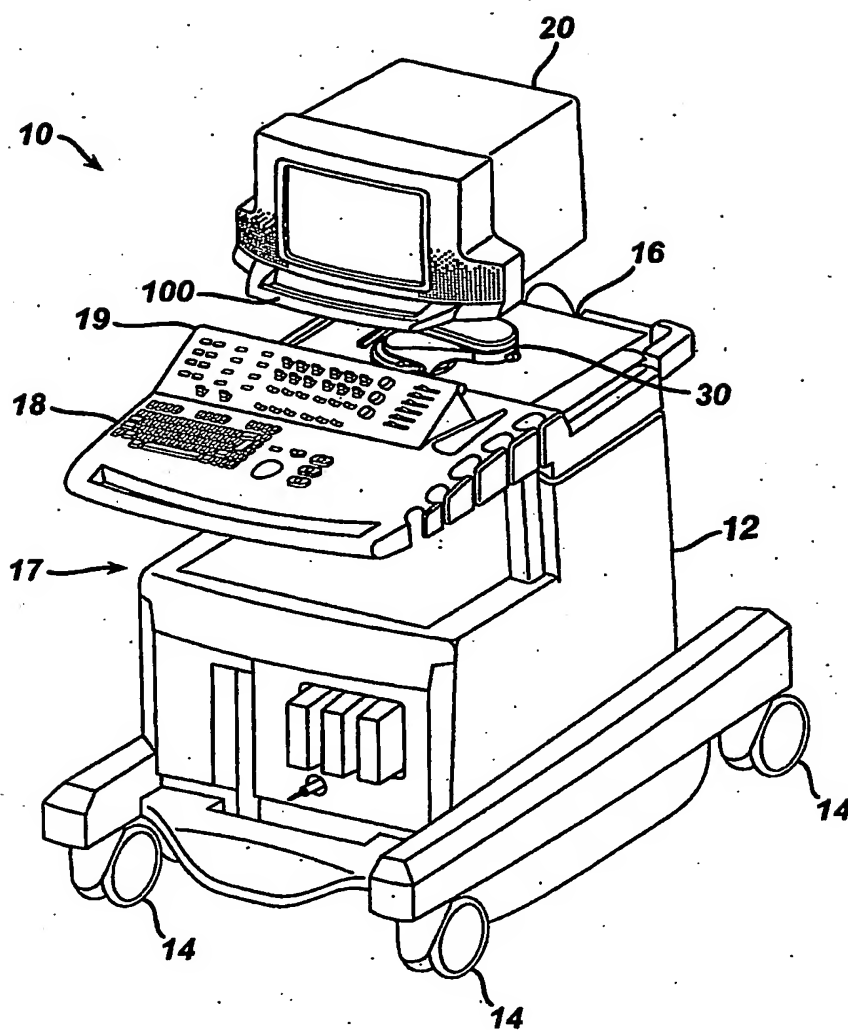


**FIG. 2**

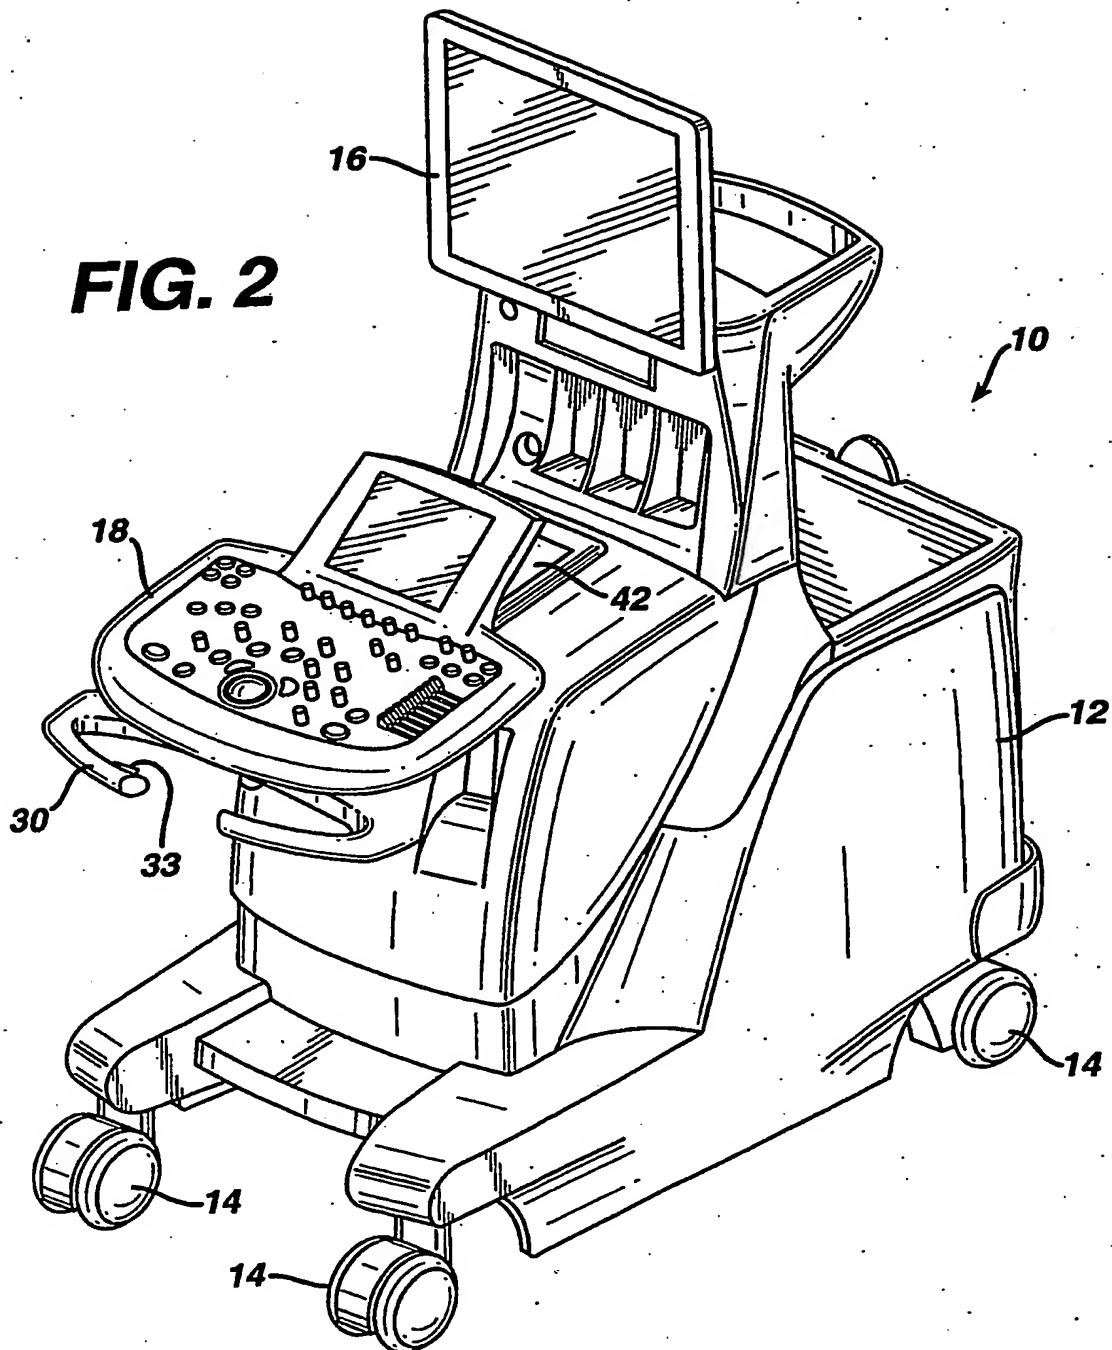


**FIG. 3**

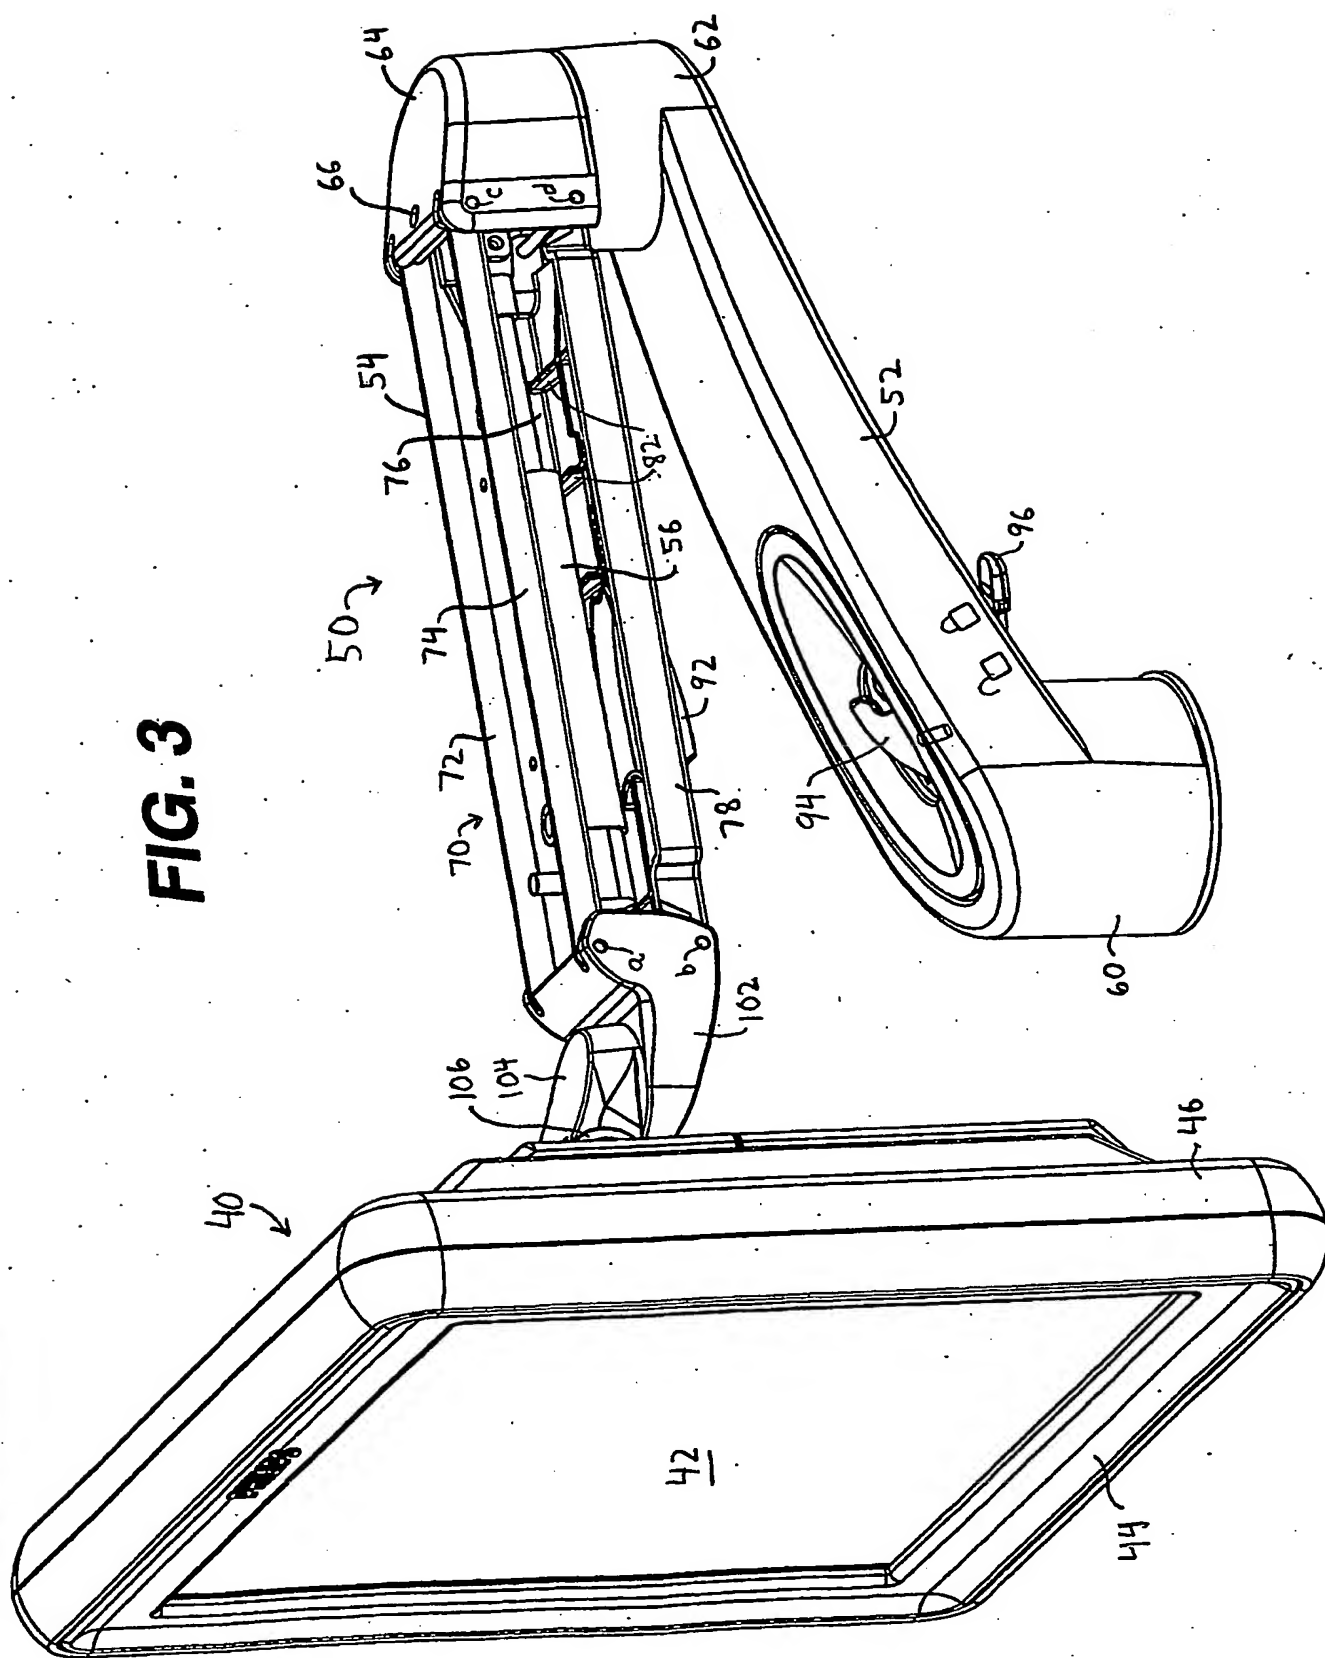

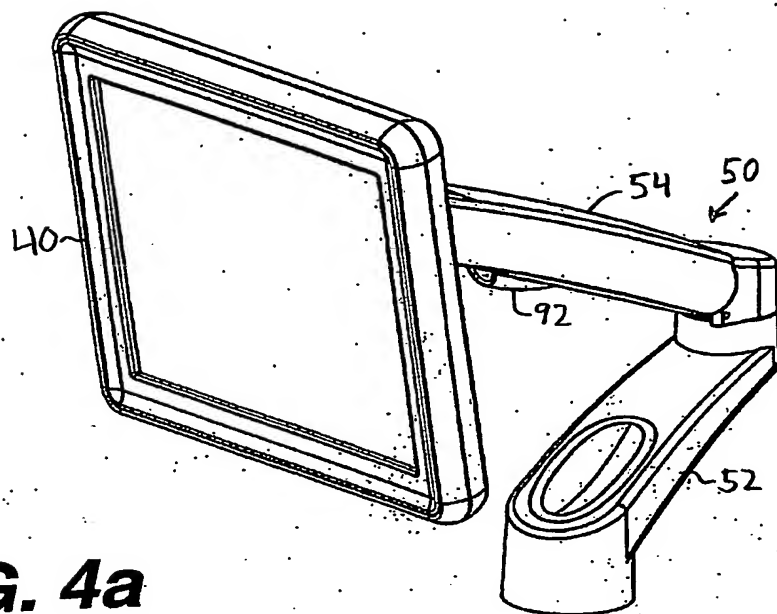


**FIG. 4a**

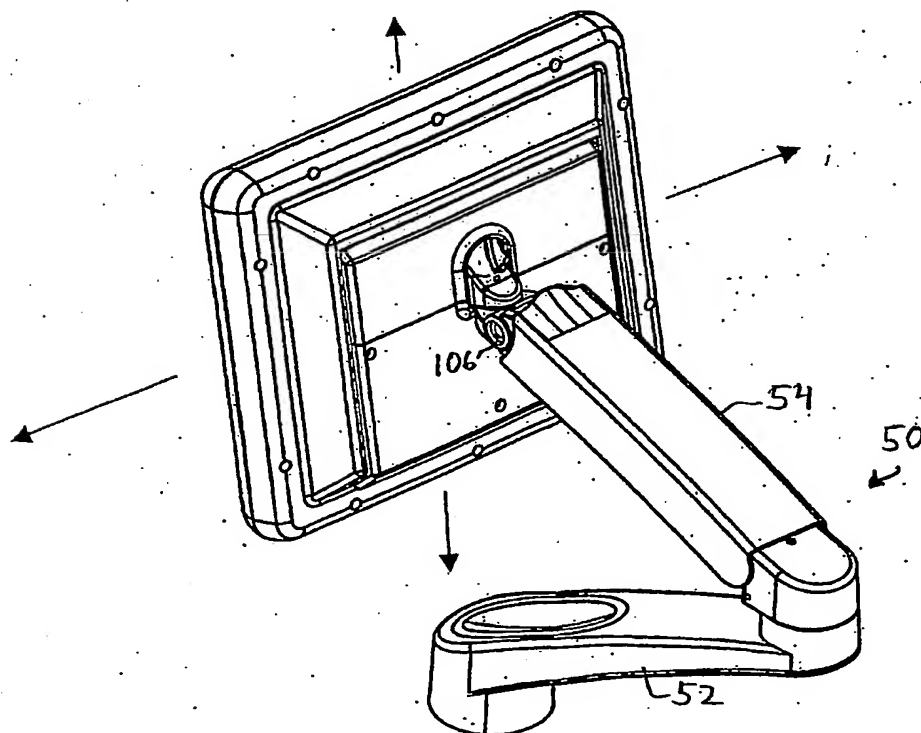


**FIG. 4b**




**FIG. 5**

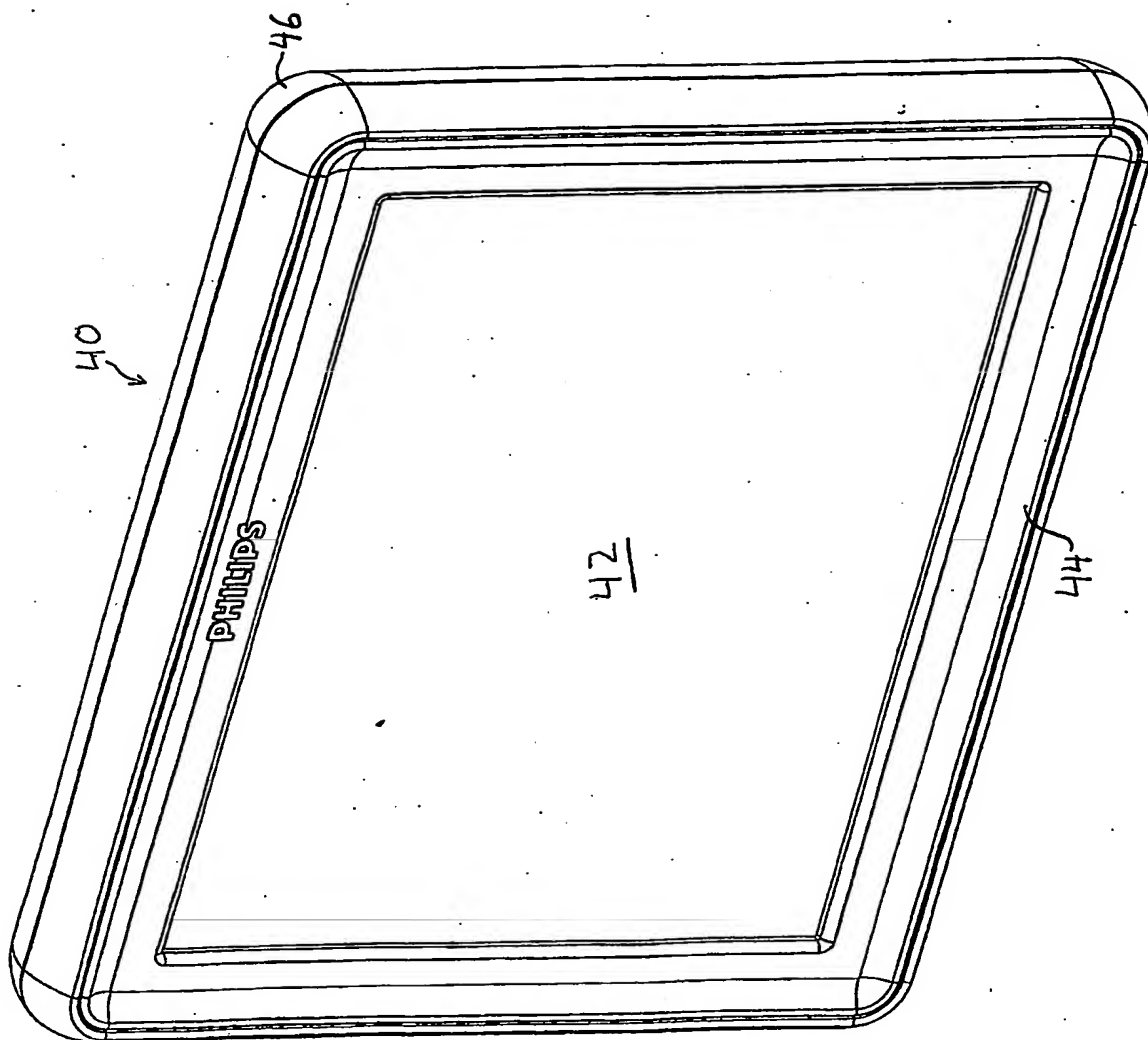


**FIG. 6**

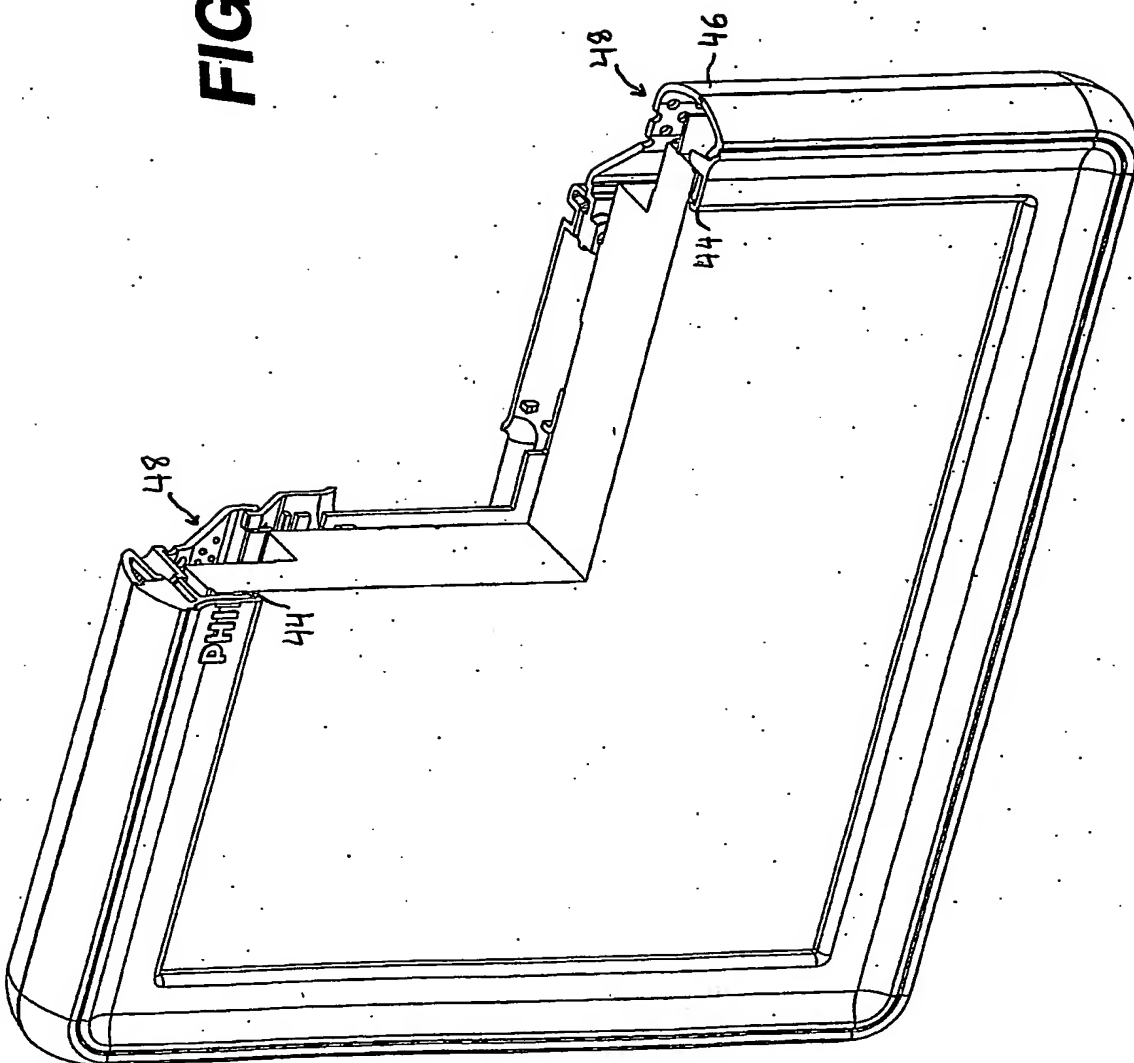


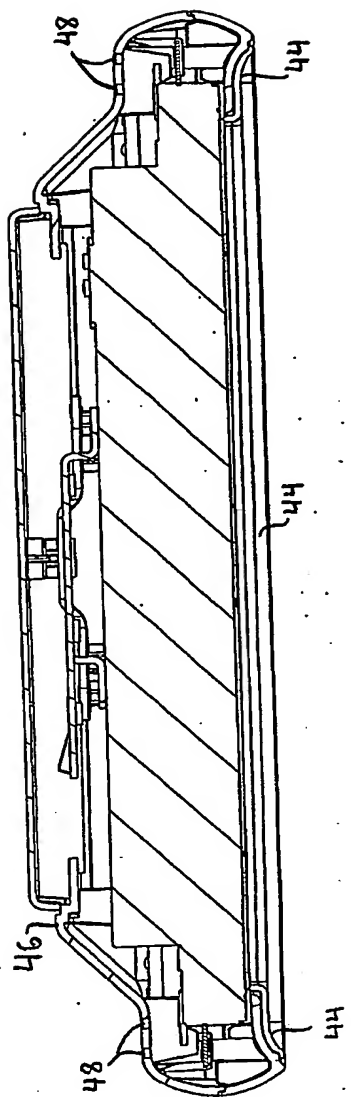


**FIG. 7a**

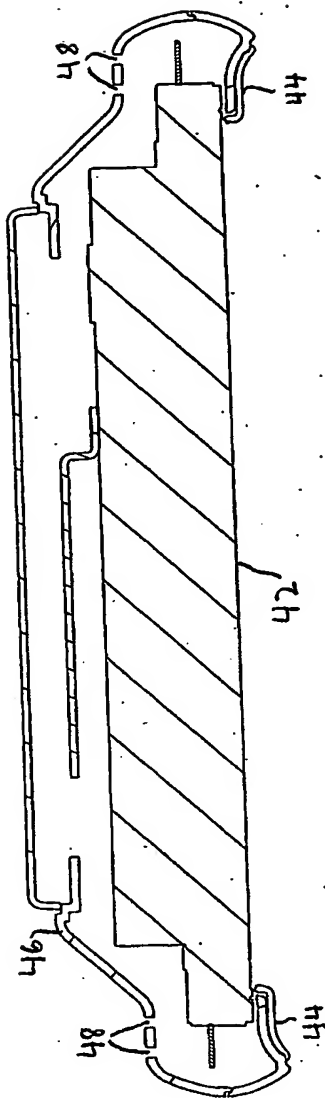


**FIG. 7b**

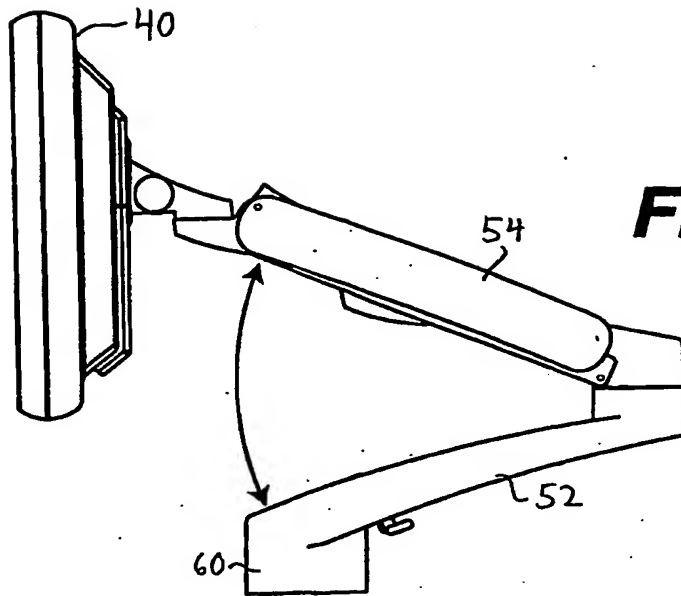


**FIG. 8a**

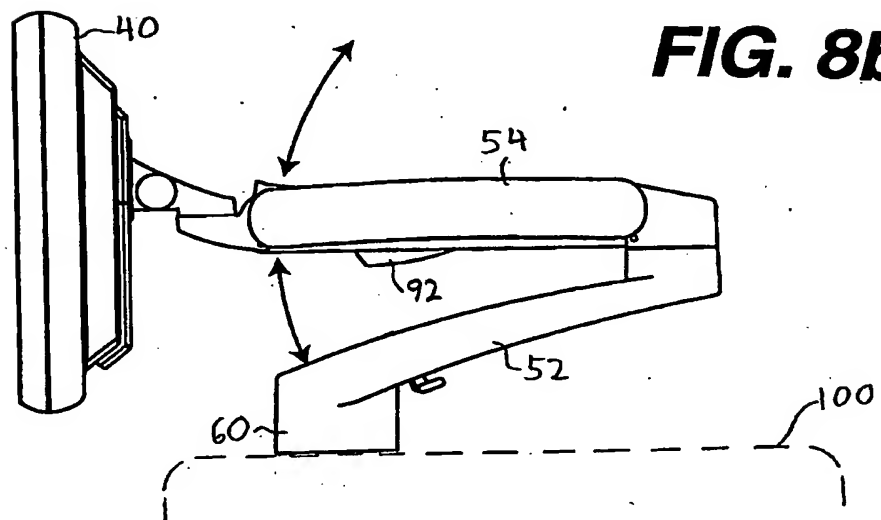

**FIG. 8b**

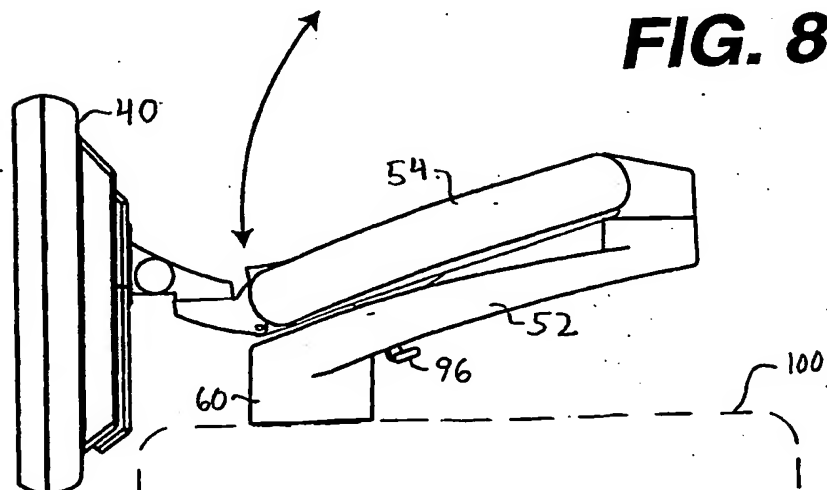


**FIG. 8c**

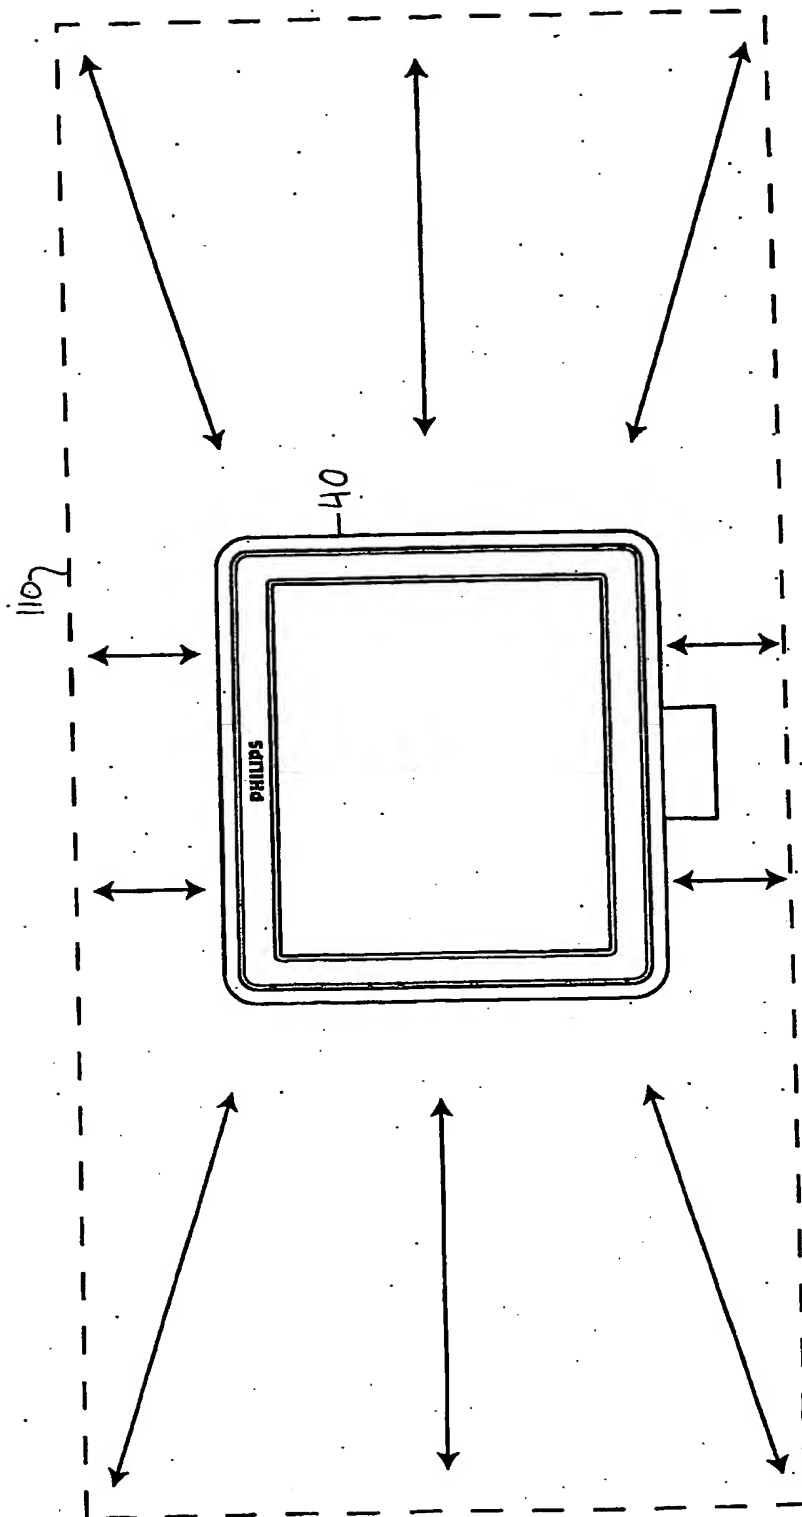


**FIG. 9**


**FIG. 10a**

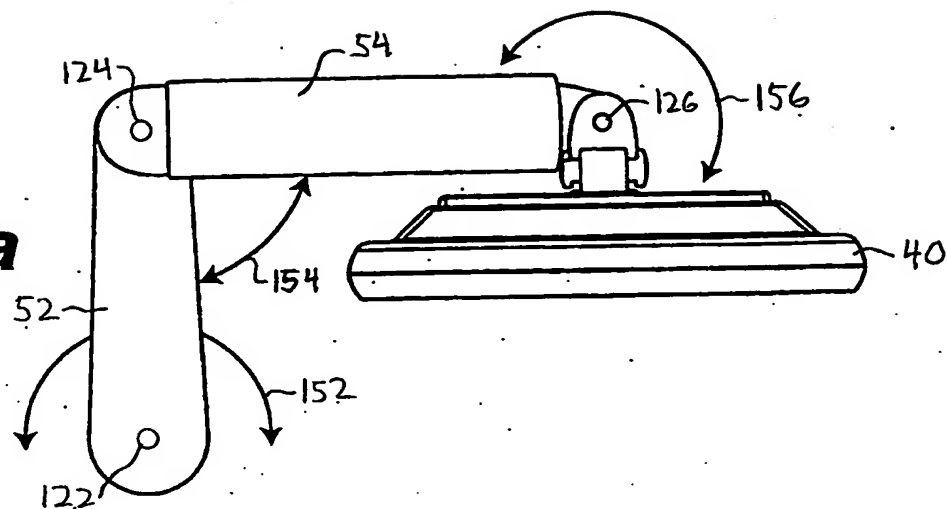


**FIG. 10b**

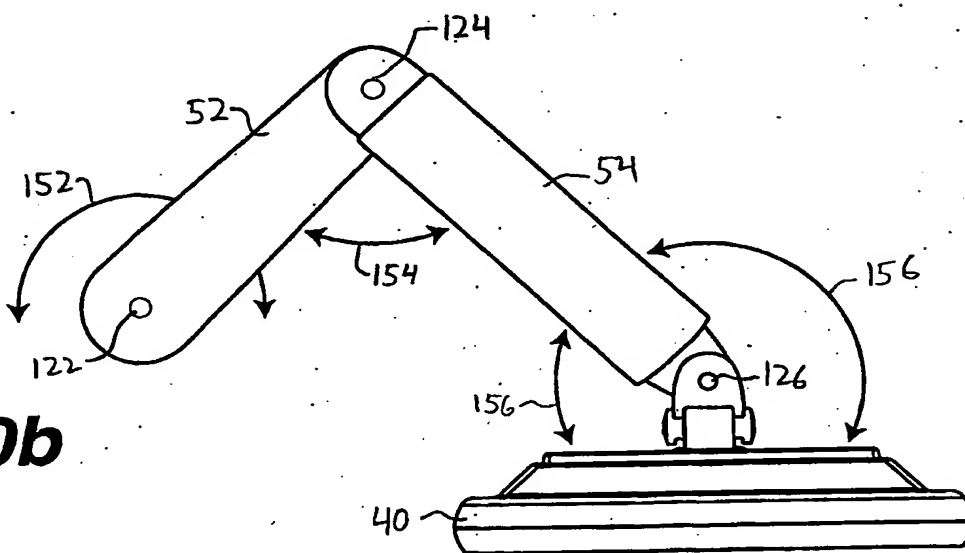

**FIG. 10c**

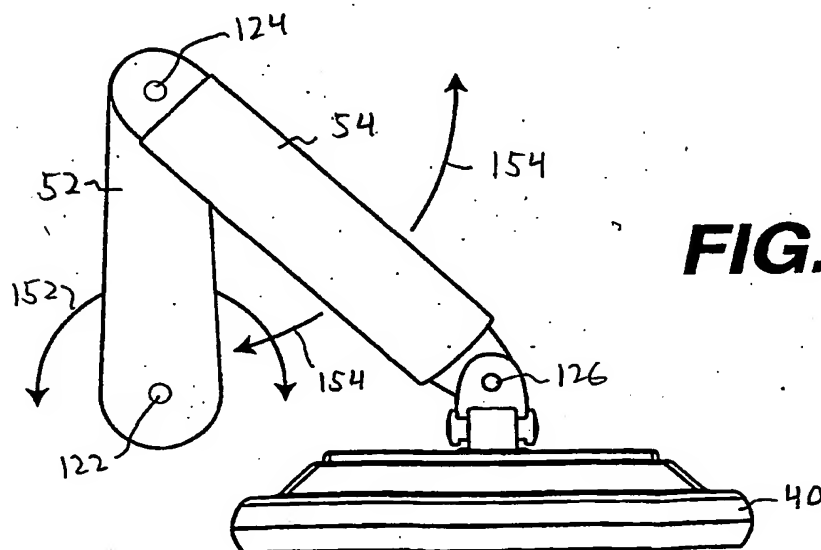

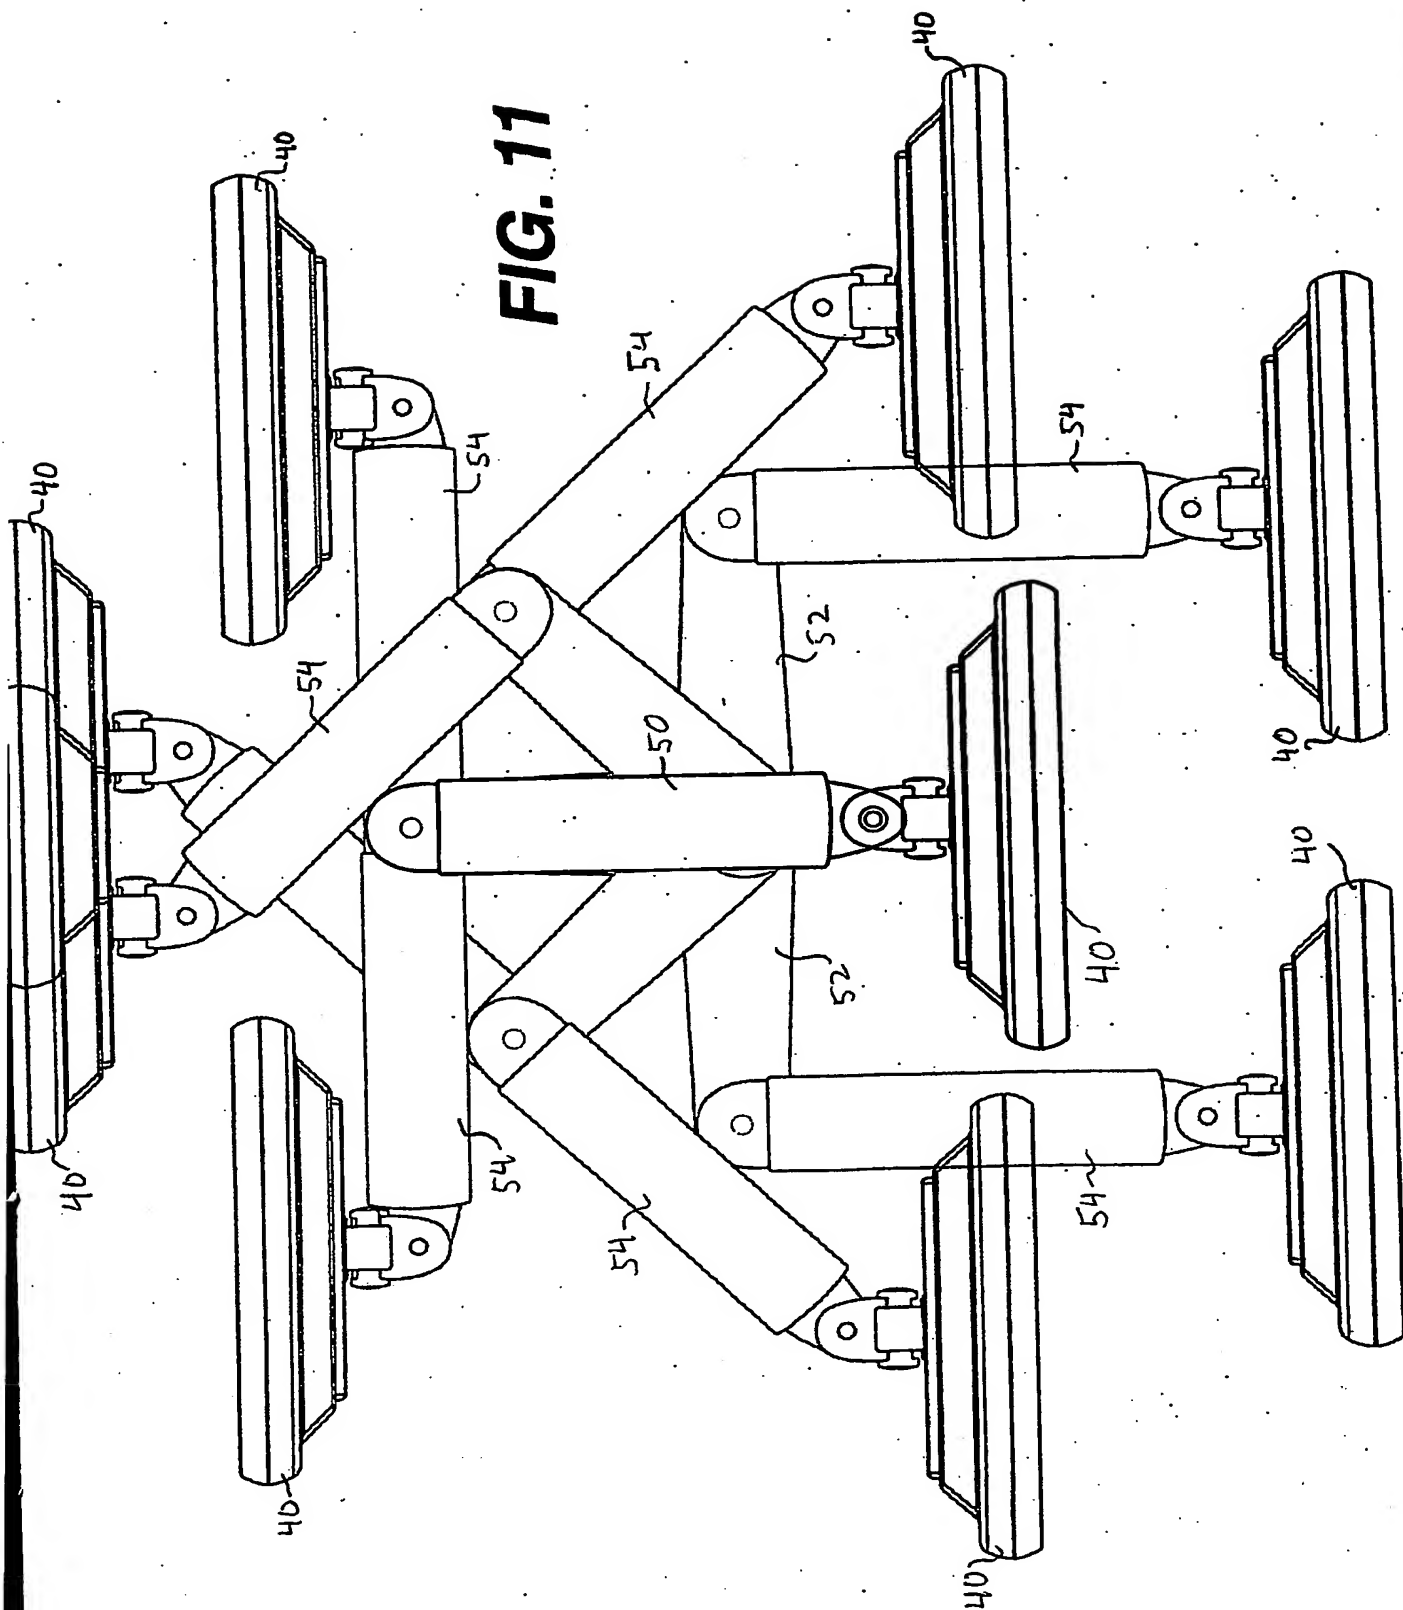

BEST AVAILABLE COPY

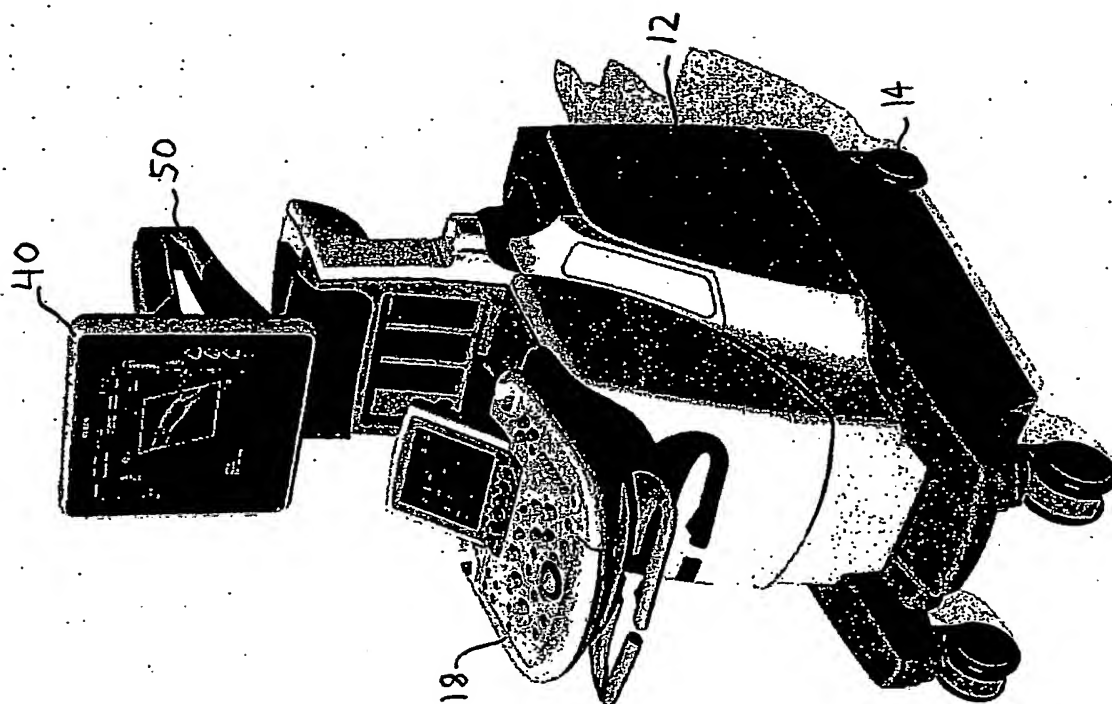


FIG. 12